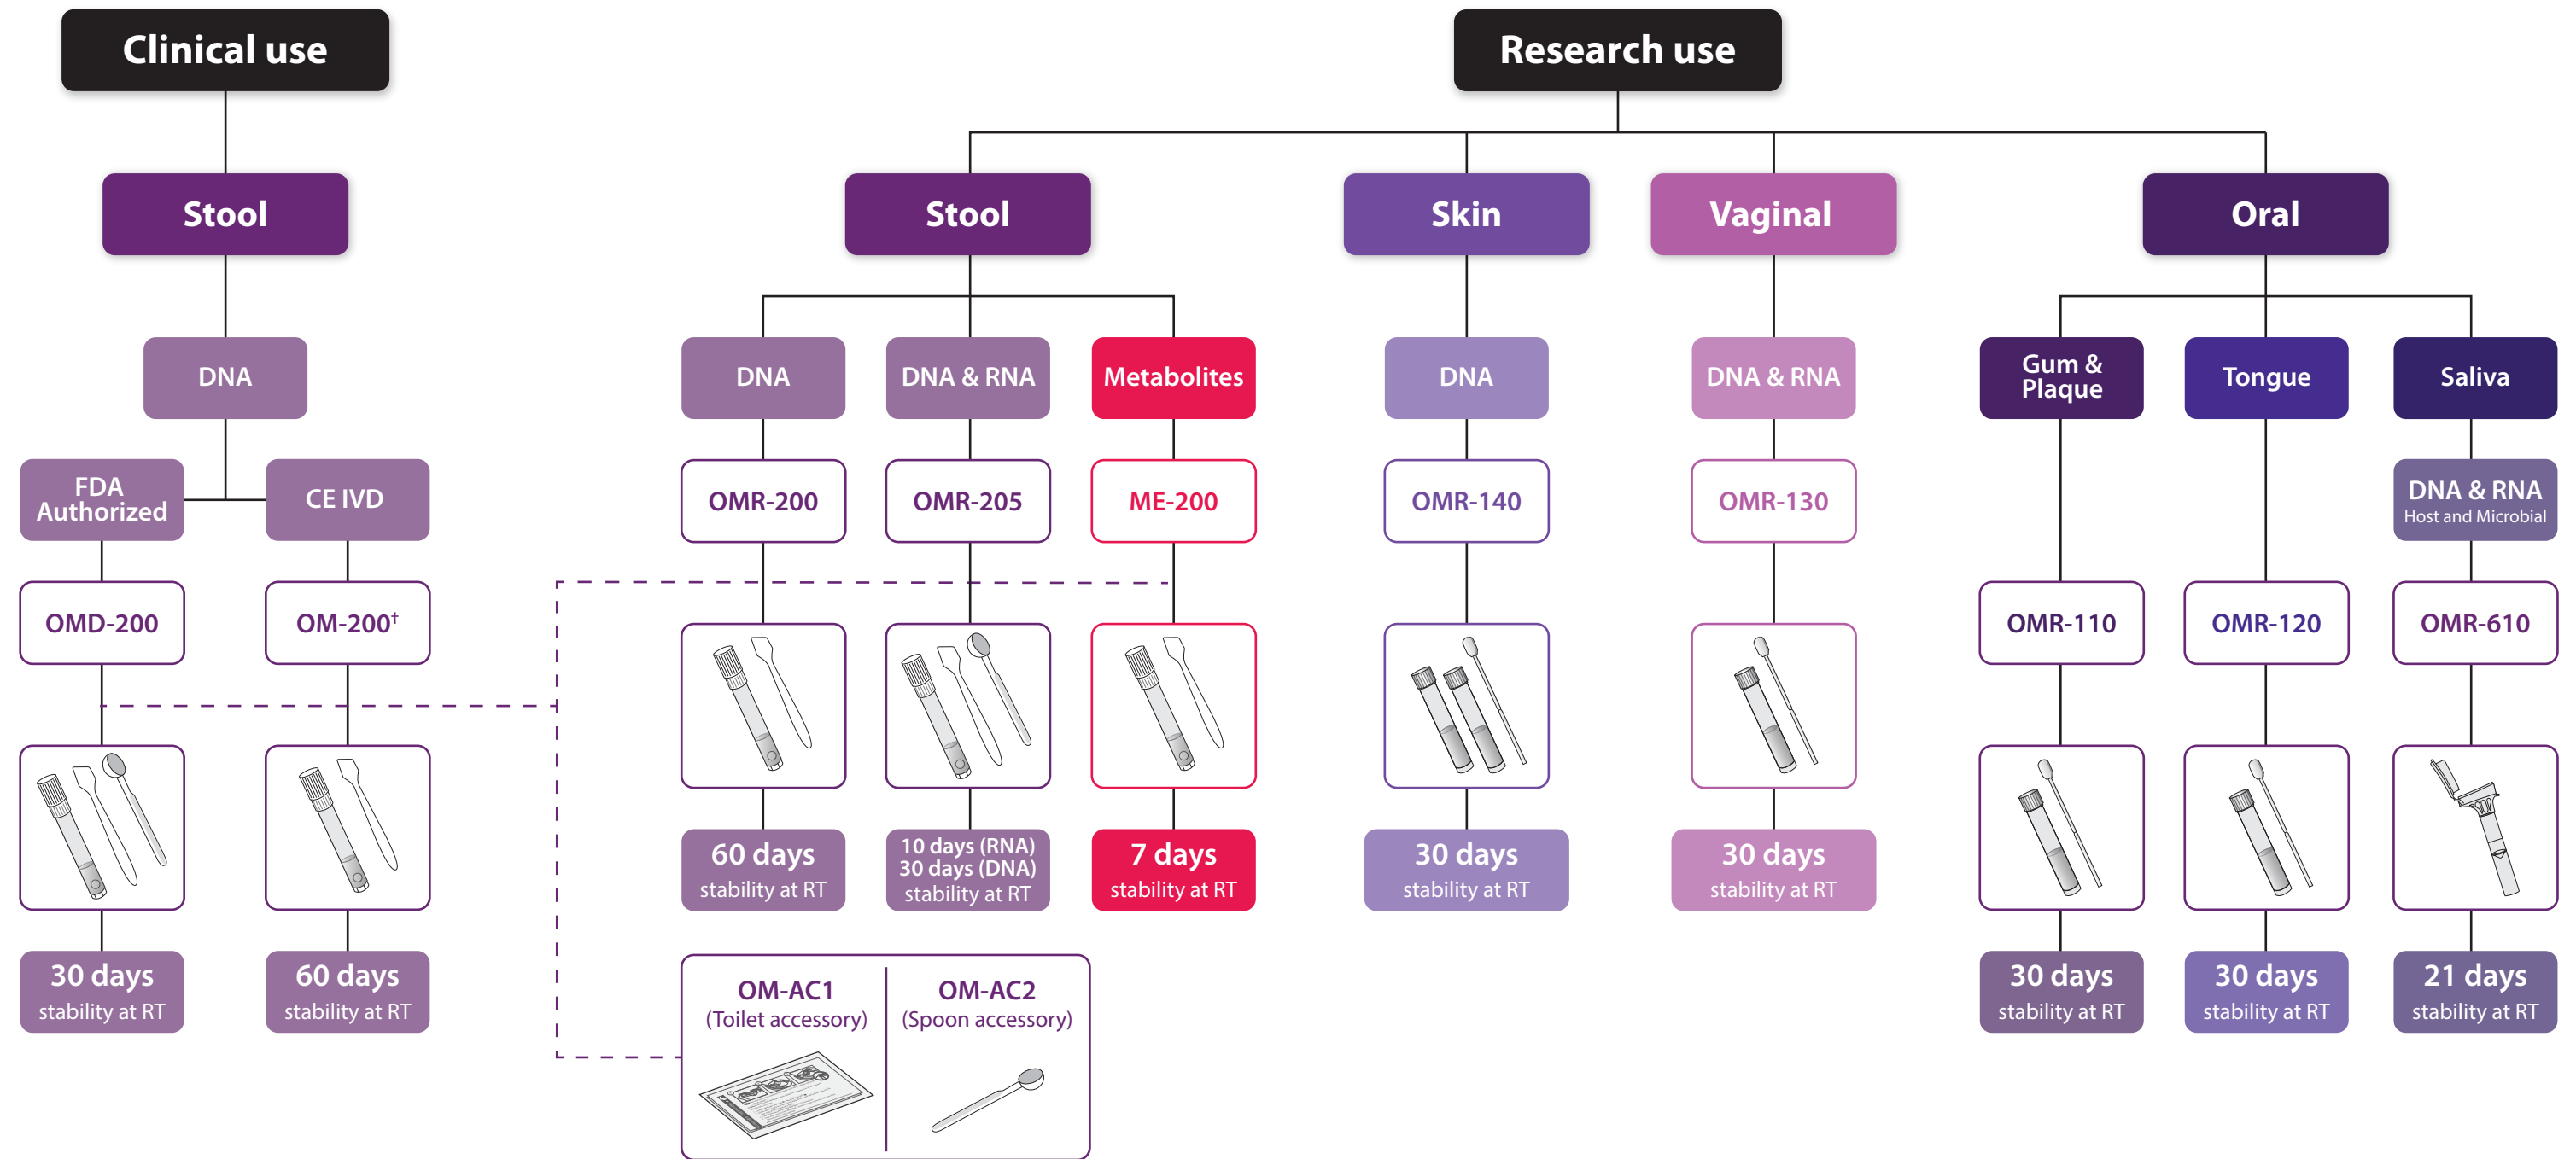


# Microbiome and metabolomics products



Some DNA Genotek products may not be available in all geographic regions.

\*OMNIgene<sup>®</sup>-GUT Dx (OMD-200) has been granted FDA De Novo classification for in vitro diagnostic use (DEN200040).

†OMNIgene<sup>®</sup>-GUT (OM-200) is CE marked For In Vitro Diagnostic Use and not available for sale in the United States.

OMNIgene<sup>®</sup>-GUT (OMR-200), OMNIgene<sup>®</sup>-ORAL (OMR-110/120), OMNIgene<sup>®</sup>-VAGINAL, OMNIgene<sup>®</sup>-SALIVA (OMR-610) and OMNIgene<sup>®</sup>-SKIN are for Research Use Only, not for use in diagnostic procedures.









OMNIgene, OMNImet and DNA Genotek are trademarks of DNA Genotek Inc.

Patent ([www.dnagenotek.com/legalnotices](http://www.dnagenotek.com/legalnotices))

© 2022 DNA Genotek Inc. is a subsidiary of OraSure Technologies, Inc., all rights reserved.

MK-01802 Issue 3/2022-12

# Microbiome and metabolomics product details

	Stool OMD-200 (DNA)	Stool OMR-205 (DNA & RNA)	Vaginal OMR-130 (DNA & RNA)	Tongue OMR-120 (DNA & RNA)	Gum & Plaque OMR-110 (DNA & RNA)	Skin OMR-140 (DNA)	Saliva OMR-610 (DNA & RNA)	Stool ME-200 (Metabolites)
								
Tare weight for collected sample (weight of tube, cap, chemistry and swab, if applicable)	13.69 g	13.69 g	5.33 g	5.33 g	5.33 g	5.62 g	6.04 g	13.77 g
Volume of chemistry	2 mL	2ml	1 mL	1 mL	1 mL	1 mL	1 mL	2.8 mL
Volume of sample collected	0.4-0.5 mL	0.4-0.5 ml	Not applicable	Not applicable	Not applicable	Not applicable	1 mL	0.4-0.5 mL
Mean (median) DNA yield/ extraction <sup>1</sup>	9.89 +/- 0.23 ug (8.72)	4.40 +/- 0.52 ug (2.06)	4.29 ± 1.15 µg (2.63 µg)	0.29 ± 0.035 µg (0.297 µg)	0.374 ± 0.036 µg (0.345 µg)	Collection site dependent	1.22 ± 0.12 ug (0.86 ug)	--
Ambient temperature sample stability <sup>2</sup>	30 days	10 days (RNA) and 30 days (DNA)	30 days	30 days	30 days	30 days	21 days	7 days <sup>3</sup>

DNA Genotek products are compatible with a wide range of extraction kits.

Please consult the specific product page or contact technical support ([support@dnagenotek.com](mailto:support@dnagenotek.com)) for additional sample processing protocols and recommendations.

<sup>1</sup> Extraction from a 250 l aliquot.

<sup>2</sup> Storage recommendations for samples collected with OMNIgene<sup>®</sup> products from DNA Genotek<sup>®</sup>. DNA Genotek. PD-PR-01036

<sup>3</sup> Storage recommendations for samples collected with OMNImet.GUT. DNA Genotek. PD-PR-00987