




ORAc collect•Dx Automation Guide

The following illustration serves as a guide for automated DNA extraction from the ORAc collect•Dx (OCD-100A) saliva collection device, featuring rapid sample recovery upon decapping.

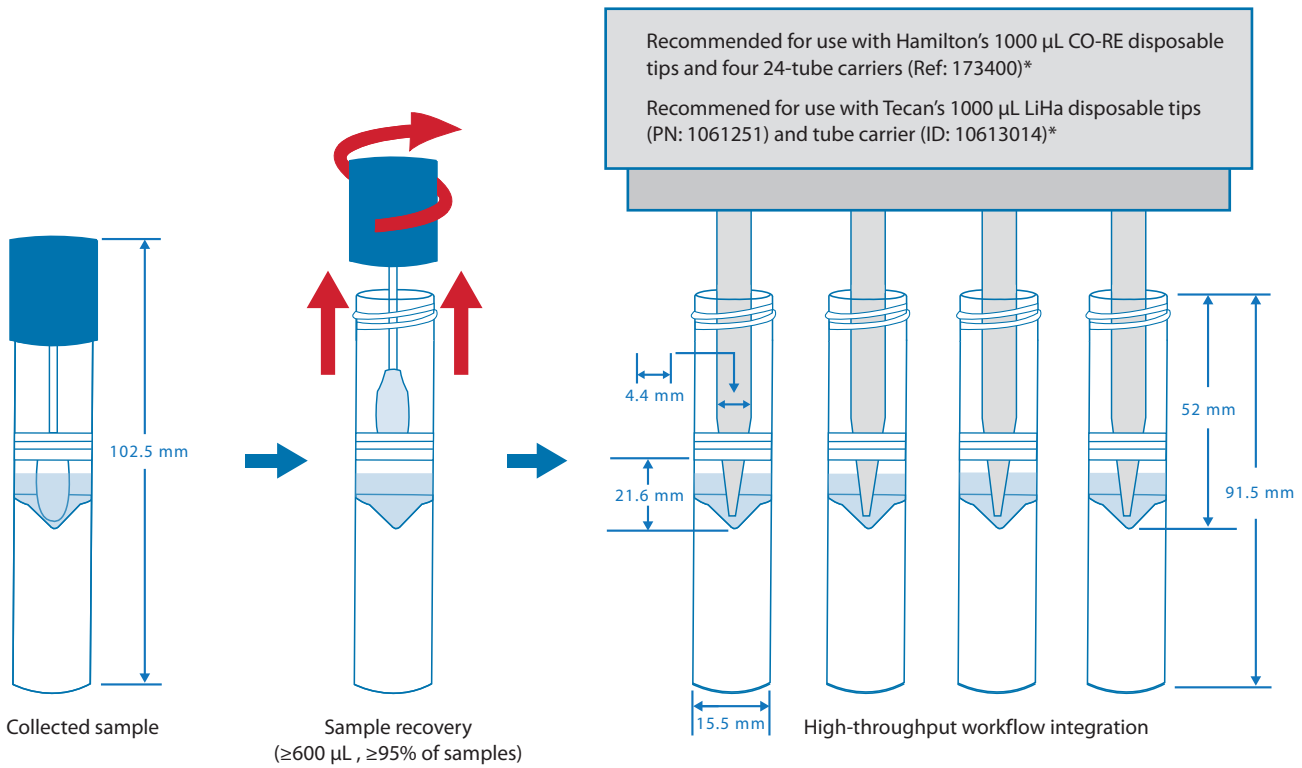

RC-2 tube replacement caps are available as an accessory item for storage of any remaining samples if required.

ORAc collect•Dx has been cleared for In Vitro diagnostic use in the USA and FDA cleared for In Vitro diagnostic use with eSensor Warfarin Sensitivity Saliva Test.
 *ORAc collect is a registered trademark of DNA Genotek Inc.
 * Reference and part numbers are not for DNA Genotek products. All other brands and names contained herein are the property of their respective owners.
 Patent (www.dnagenotek.com/legalnotices)

For In Vitro Diagnostic Use
CE
 For collection of human DNA

DNA Genotek Inc.
 3000 - 500 Palladium Drive
 Ottawa, ON, Canada K2V 1C2
 Subsidiary of OraSure Technologies, Inc.

Toll-free (North America): 1.866.813.6354
 Tel.: +1.613.723.5757 • Fax: +1.613.723.5057
 www.dnagenotek.com
 info@dnagenotek.com

DNAgenotek

Superior samples • Proven performance